


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-N05-4625	Mobile Phase:	n-Hexane:IPA=99.5:0.5
Serial No:	H22073010	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu NH <sub>2</sub> 5μm	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	10μl
Pressure:	40bar	Sample:	Nitrobenzene

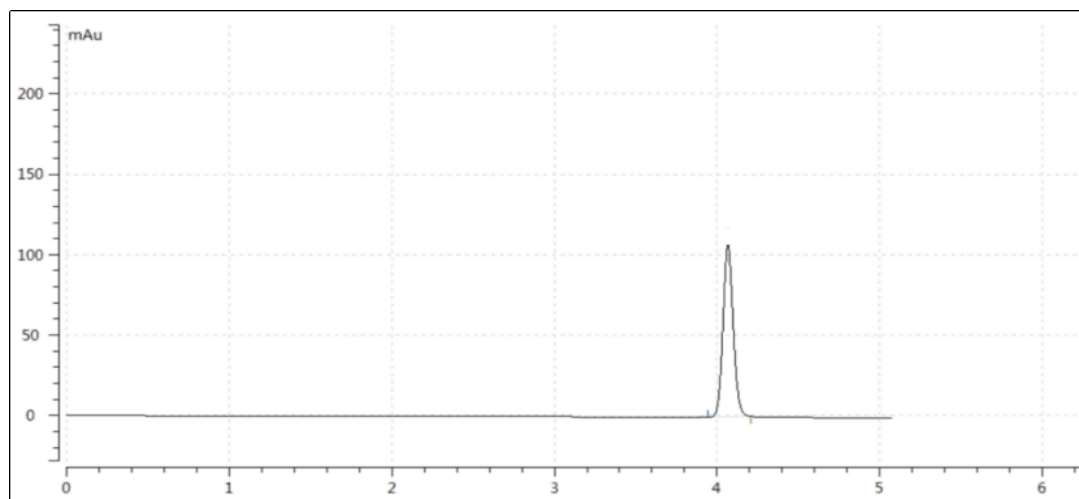

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N)
1	Nitrobenzene	4.139	1.01	20637

Test Result: Qualified

