


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-F03-2105	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22072701	Flow Rate:	0.2ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu PFP 3 μ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	0.2 μ l
Pressure:	63bar	Sample:	Naphthalene

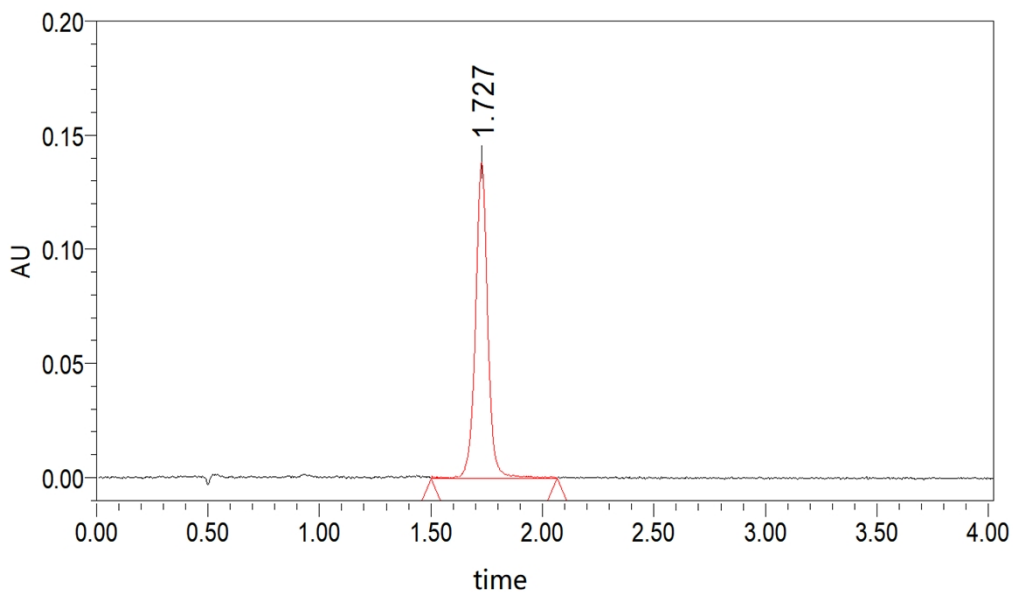

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Naphthalene	1.727	1.01	5310

Test Result: Qualified

