


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-F03-2105	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22072702	Flow Rate:	0.2ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu PFP 3 $\mu$ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	0.2 $\mu$ l
Pressure:	62bar	Sample:	Naphthalene

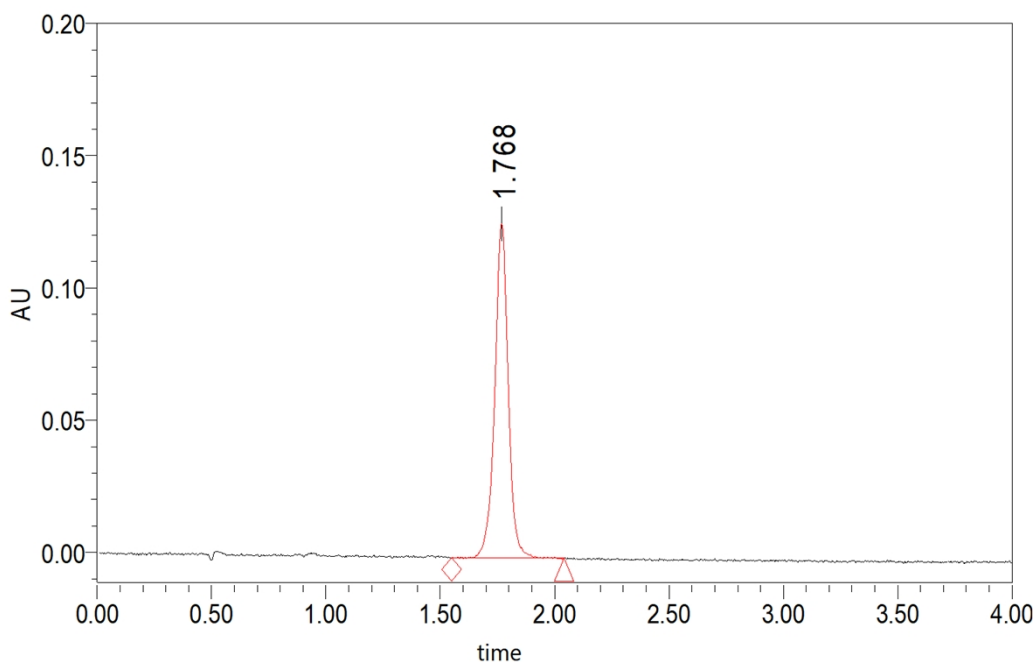

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Naphthalene	1.768	0.98	4952

Test Result: Qualified

