


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BS05-4625	Mobile Phase:	ACN:H ₂ O=70:30
Serial No:	H22033106	Flow Rate:	1.0ml/min
Batch No:	S02050-J01-011001	Temperature:	Ambient
Bulk Material:	Hungpu ST C18 5μm	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5μl
Pressure:	7.1MPa	Sample:	Acetone、Acenaphthene

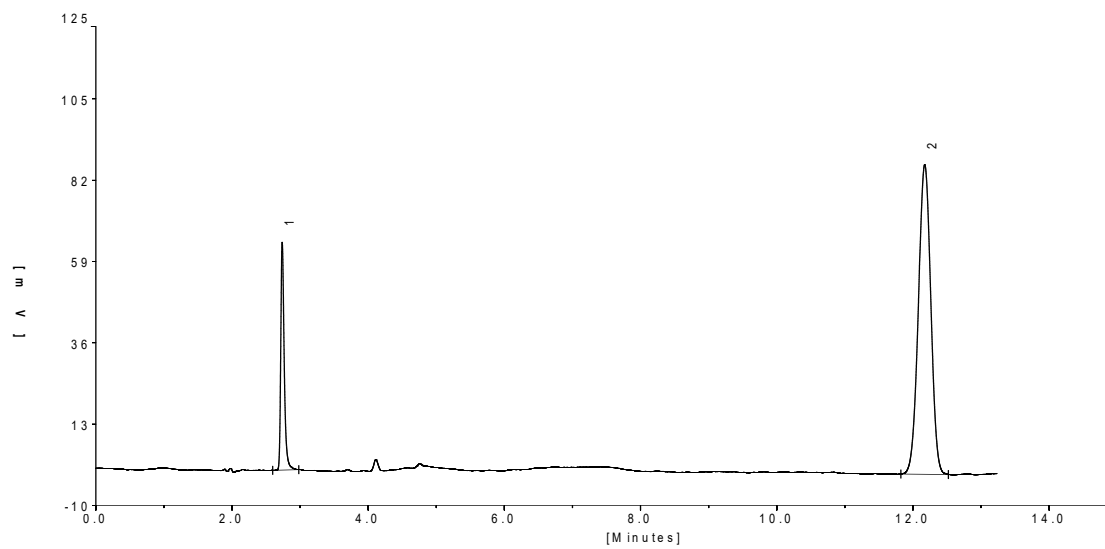

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.73	1.40	62209
2	Acenaphthene	12.17	0.98	84200

Test Result: Qualified

