


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Ca08-7830	Mobile Phase:	Water
Serial No:	H22071901	Flow Rate:	0.6ml/min
Batch No:	H2201A	Temperature:	80°C
Bulk Material:	Hungpu Sugar-Ca 8μm	Detector:	UV
Dimensions:	300*7.8mm	Injection Volume:	50μl
Pressure:	26bar	Sample:	Acetone

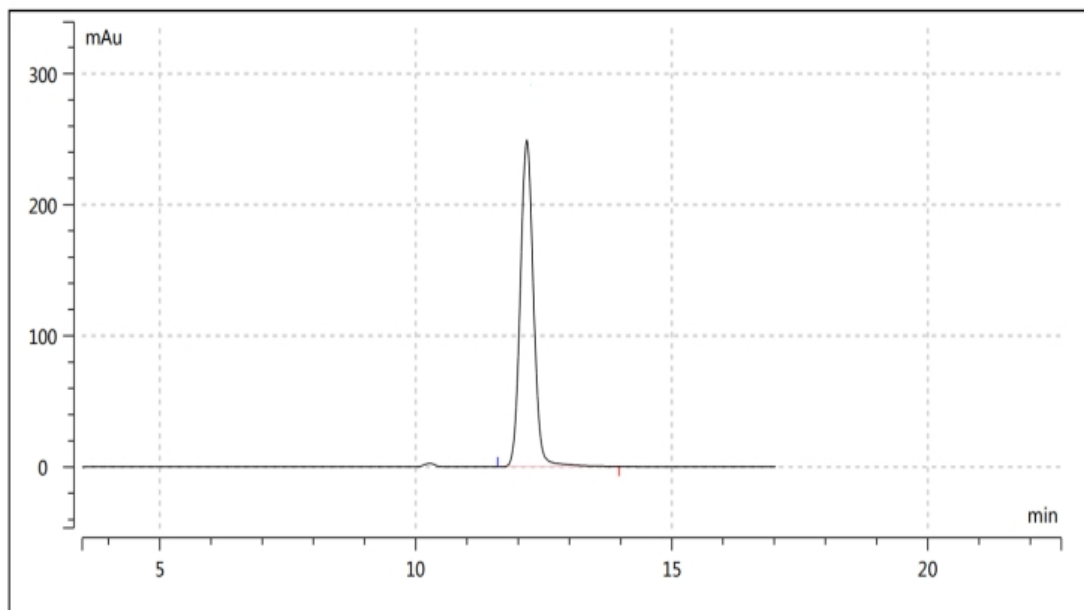

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency
1	Acetone	12.637	0.98	8900

Test Result: Qualified

