


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BA03-4610	Mobile Phase:	ACN:H2O=75:25
Serial No:	H22072104	Flow Rate:	0.8ml/min
Batch No:	D02030-J10-011001	Temperature:	Ambient
Bulk Material:	Hungpu T3 3 $\mu$ m	Detector:	254nm
Dimensions:	100*4.6mm	Injection Volume:	5 $\mu$ l
Pressure:	5.6Mpa	Sample:	Acetone、Acenaphthene

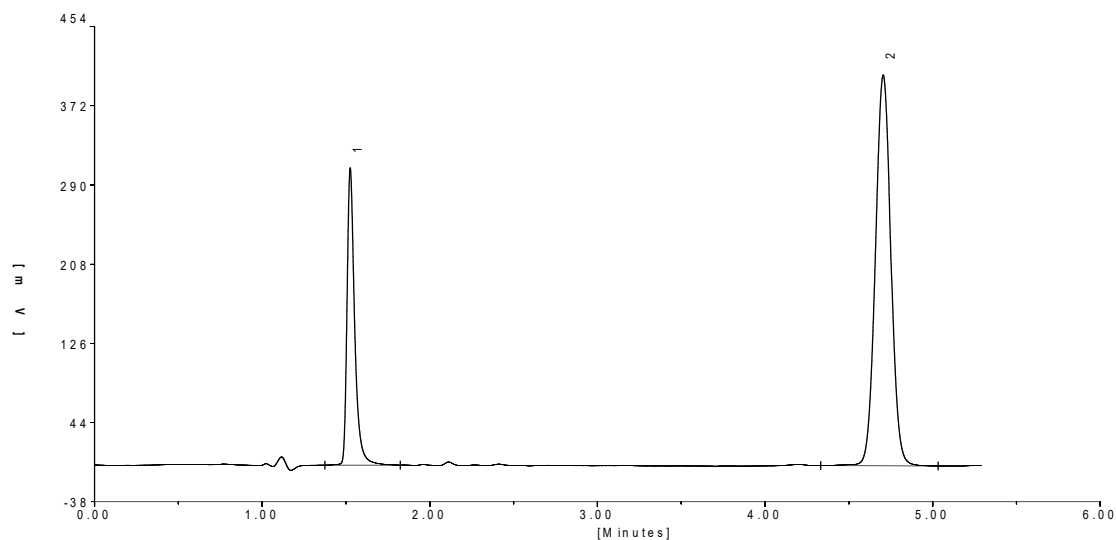

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	1.52	1.47	61398
2	Acenaphthene	4.70	1.03	126831

Test Result:Qualified

