


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX02-2110	Mobile Phase:	ACN:H <sub>2</sub> O=60:40
Serial No:	H22071401	Flow Rate:	0.2ml/min
Batch No:	H02020-J06-011001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 2μm	Detector:	254nm
Dimensions:	100*2.1mm	Injection Volume:	1μl
Pressure:	3681PSi	Sample:	Acetone、Acenaphthene

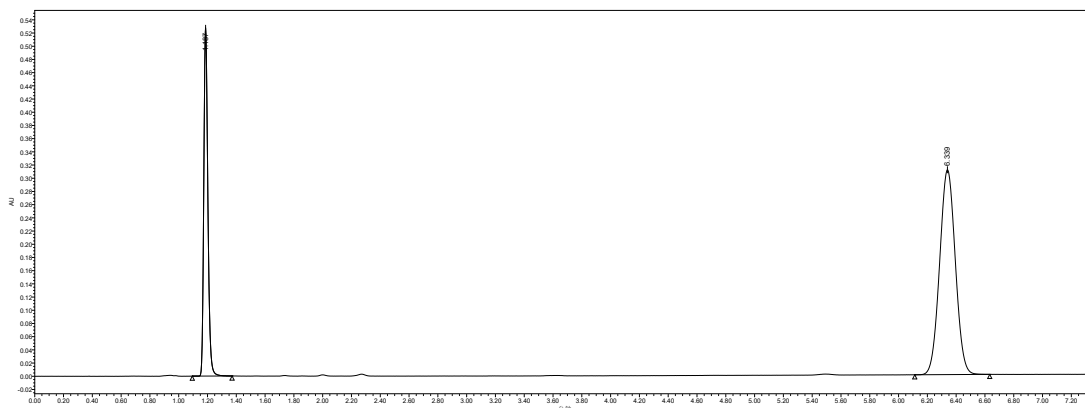

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	1.18	1.24	87440
2	Acenaphthene	6.33	1.03	165200

Test Result:Qualified

