


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX03-4610	Mobile Phase:	ACN:H <sub>2</sub> O=70:30
Serial No:	H22071606	Flow Rate:	0.8ml/min
Batch No:	H02030-J06-012001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 3μm	Detector:	254nm
Dimensions:	100*4.6mm	Injection Volume:	5μl
Pressure:	6.8MPa	Sample:	Acetone、Acenaphthene

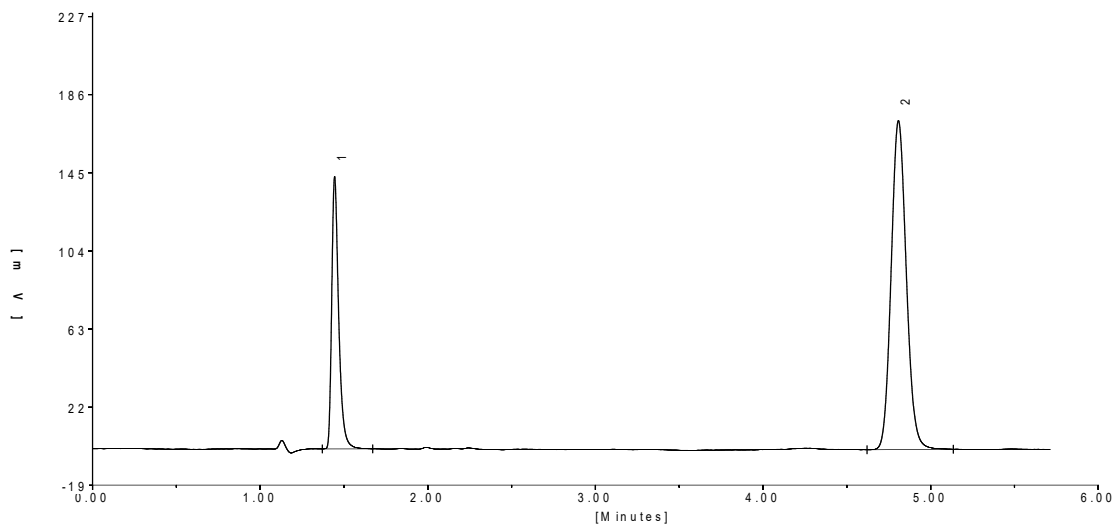

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	1.44	1.44	64042
2	Acenaphthene	4.80	1.10	137023

Test Result: Qualified

