


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-4615	Mobile Phase:	ACN:H ₂ O=70:30
Serial No:	H22072703	Flow Rate:	0.8ml/min
Batch No:	H02050-J06-012001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 5μm	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5μl
Pressure:	3.4MPa	Sample:	Acetone、Acenaphthene

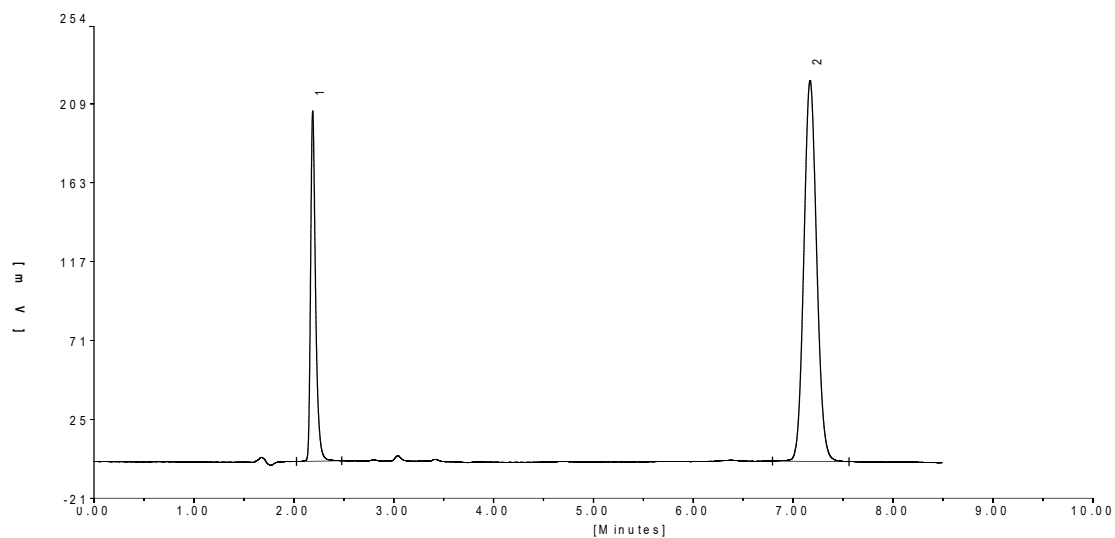

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.18	1.42	70800
2	Acenaphthene	7.16	1.09	99174

Test Result: Qualified

