


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-4615	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22073101	Flow Rate:	0.8ml/min
Batch No:	H02050-J06-012001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 5 μ m	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5 μ l
Pressure:	3.3MPa	Sample:	Acetone、Acenaphthene

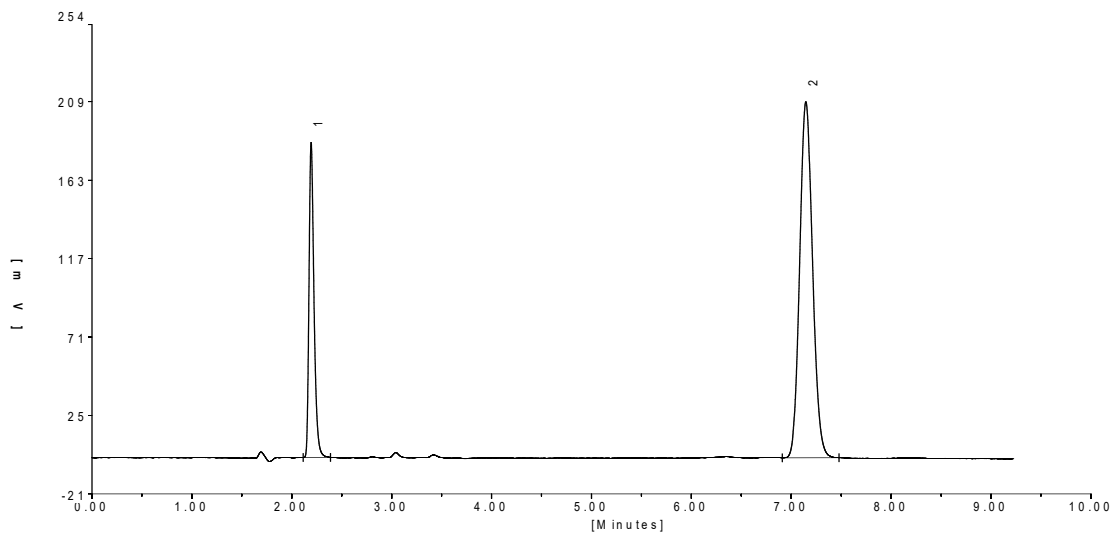

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.19	1.39	64462
2	Acenaphthene	7.14	1.10	98553

Test Result:Qualified

