


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX02-0303	Mobile Phase:	ACN:H <sub>2</sub> O=50:50
Serial No:	H22072416	Flow Rate:	0.6ml/min
Batch No:	H02020-J10-011001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 2 $\mu$ m	Detector:	254nm
Dimensions:	30*3.0mm	Injection Volume:	1 $\mu$ l
Pressure:	2173Psi	Sample:	Acetone、Acenaphthene

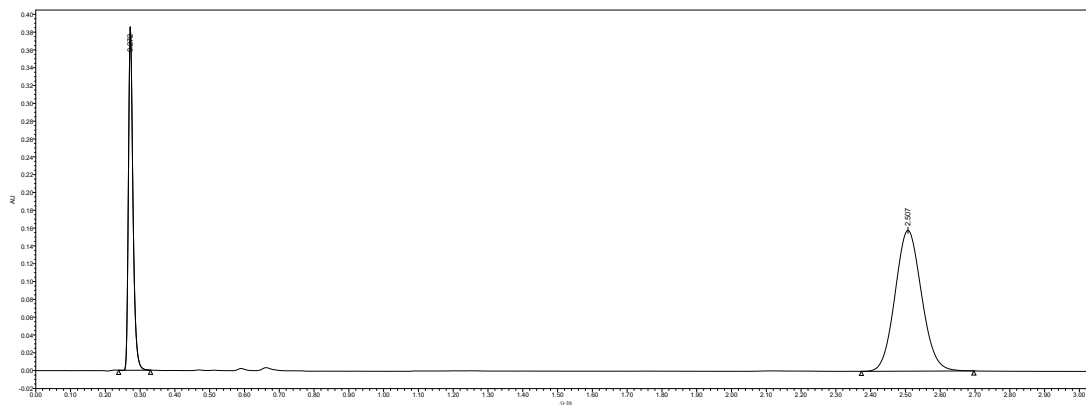

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.27	1.36	70158
2	Acenaphthene	2.50	1.07	170449

Test Result:Qualified

